


Sample Name: OT 1128-001-20

```

=====
Acq. Operator   :                               Seq. Line :    4
Acq. Instrument : Instrument 1                  Location  : Vial 4
Injection Date  : 11/23/2020 1:26:26 PM        Inj       :    1
                                                Inj Volume: 1 µl

Acq. Method    : C:\CHEM32\1\DATA\PCB ADT 2020-11-23 11-59-18\PCBS.M
Last changed   : 10/16/2020 4:49:57 PM
Analysis Method: C:\CHEM32\1\METHODS\AROCLOR 1254 CUANTIF.M
Last changed   : 11/18/2020 9:03:19 AM
Method Info    : ECD checkout method.
=====
    
```

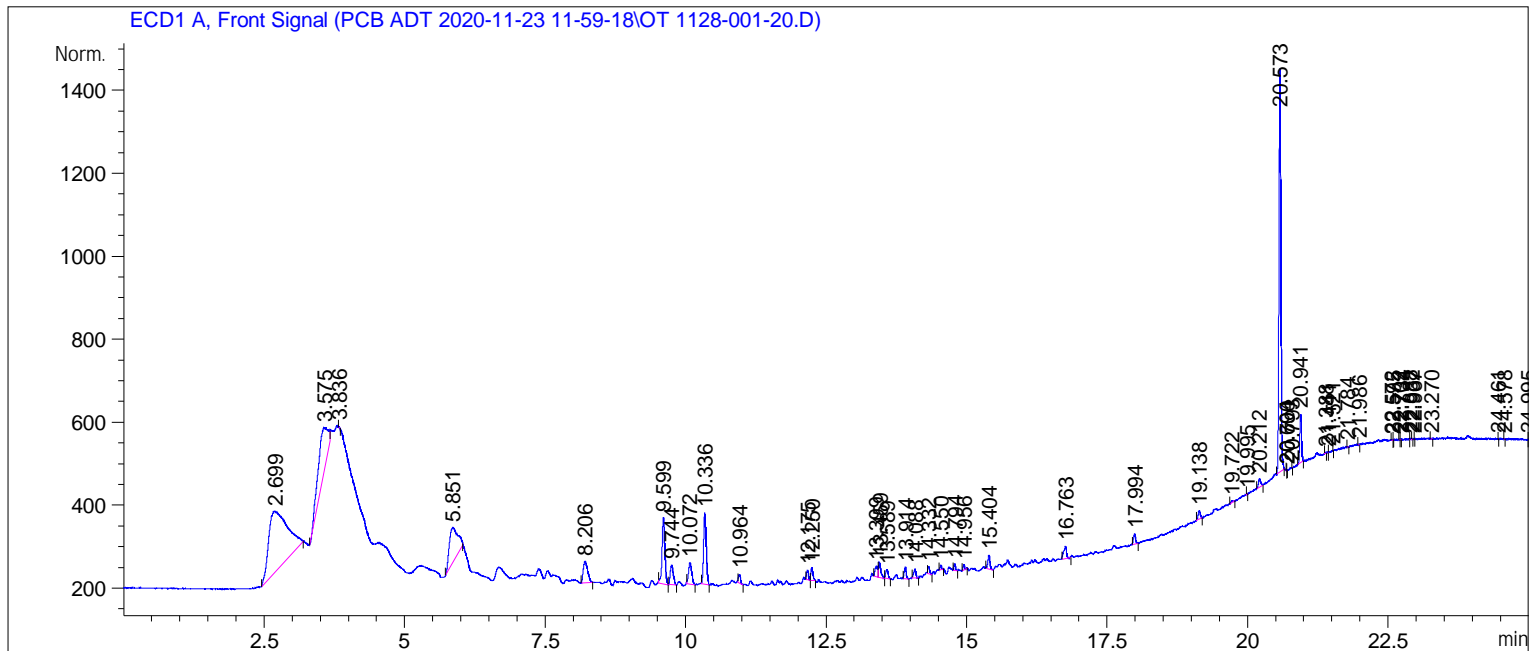

External Standard Report

```

=====
Sorted By      : Signal
Calib. Data Modified : Wednesday, November 18, 2020 8:43:58 AM
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: ECD1 A, Front Signal

RetTime [min]	Type	Area [Hz*s]	Amt/Area	Amount [ug/L]	Grp	Name
16.205	-	-	-	-	1	PCB1
16.763	BB	96.72144	1.21813e-2	1.17820	1	PCB2
17.092	-	-	-	-	1	PCB3
17.269	-	-	-	-	1	PCB4
17.748	-	-	-	-	1	PCB5

Totals : 1.17820

Group summary :

Sample Name: OT 1128-001-20

=====  
Acq. Operator : Seq. Line : 4  
Acq. Instrument : Instrument 1 Location : Vial 4  
Injection Date : 11/23/2020 1:26:26 PM Inj : 1  
 Inj Volume: 1 µl  
Acq. Method : C:\CHEM32\1\DATA\PCB ADT 2020-11-23 11-59-18\PCBS.M  
Last changed : 10/16/2020 4:49:57 PM  
Analysis Method : C:\CHEM32\1\METHODS\AROCLOR 1254 CUANTIF.M  
Last changed : 11/18/2020 9:03:19 AM  
Method Info : ECD checkout method.  
=====

=====  
Group Use Area Amount Group Name  
ID [Hz\*s] [ug/L] |-----|  
1 G 96.72144 1.17820 AROCLOR 1254

2 Warnings or Errors :

- Warning : Calibration warnings (see calibration table listing)
- Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*